



DIAGNOSTIC

Explorers	B2
Probes	B6
Explos	B13
Dressing Pliers	B16
Mirrors	B18





DIAGNOSTIC SET-UPS

EXAM SET-UP


DESCRIPTION	SUGGESTION
Cassette	IM605x*
Mirror/Handle	MIR5HD, MH6
Explorers	EXTU17/236, EXD11/126
Probe	PCP126
Dressing Pliers	DP2

PERIO EXAM SET-UP

DESCRIPTION	SUGGESTION
Cassette	IM605x*
Mirror/Handle	MIR5/3, MH6
Explorers	EXD56, EXD11/12A6
Probe	PCPUNC156, PQ2N6
Dressing Pliers	DP2

OTHER RECOMMENDED PRODUCTS:

Suction Tip, Color-Coded Rings

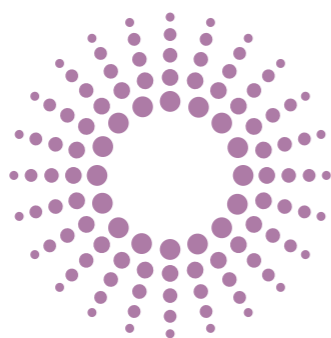

x* See Section A for exact product code number for cassette color desired.

HANDLE OPTIONS



DOUBLE END

#8 ResinEight



#7 Satin Steel Colours



#6 Satin Steel



#31 Round



SINGLE END

#8 ResinEight



#7 Satin Steel Colours



#6 Satin Steel




#30 Round



Carpal Tunnel Syndrome Prevention: Neurologists recommend alternating instrument handle sizes as one means of reducing stress. Larger diameter handles (#6, #7, #8) help lighten instrument grasp. Using a combination of various handle sizes plus a more relaxed grasp can help lessen the severity of the symptoms of Carpal Tunnel Syndrome.

Source: Gerwatowski, L.J., McFall, D.B., Stach, D.: Carpal Tunnel Syndrome; Risk Factors and Preventive Strategies for the Dental Hygienist. Journal of Dental Hygiene, February 1992.

HOW TO USE THIS SECTION

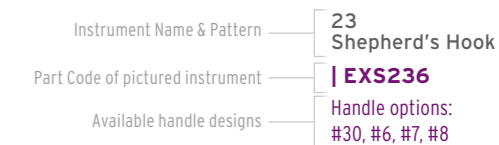


See index for all available part codes of a specific pattern.

*Do not expose resin instruments to phenols, glutaraldehydes or iodophors.



EXPLORERS


Used for caries and calculus detection, exploration of pocket characteristics, furcations and restorations.

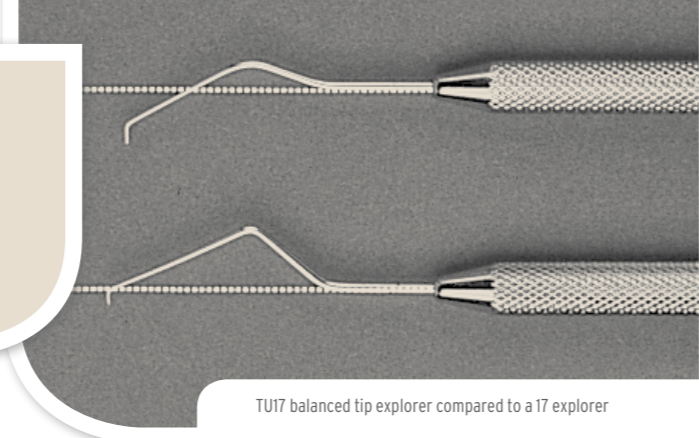

TU17 balanced tip explorer compared to a #17 explorer


SINGLE-END EXPLORERS

Satin Steel® XTS® explorers feature a non-stick Aluminum Titanium Nitride (AlTiN) coating.

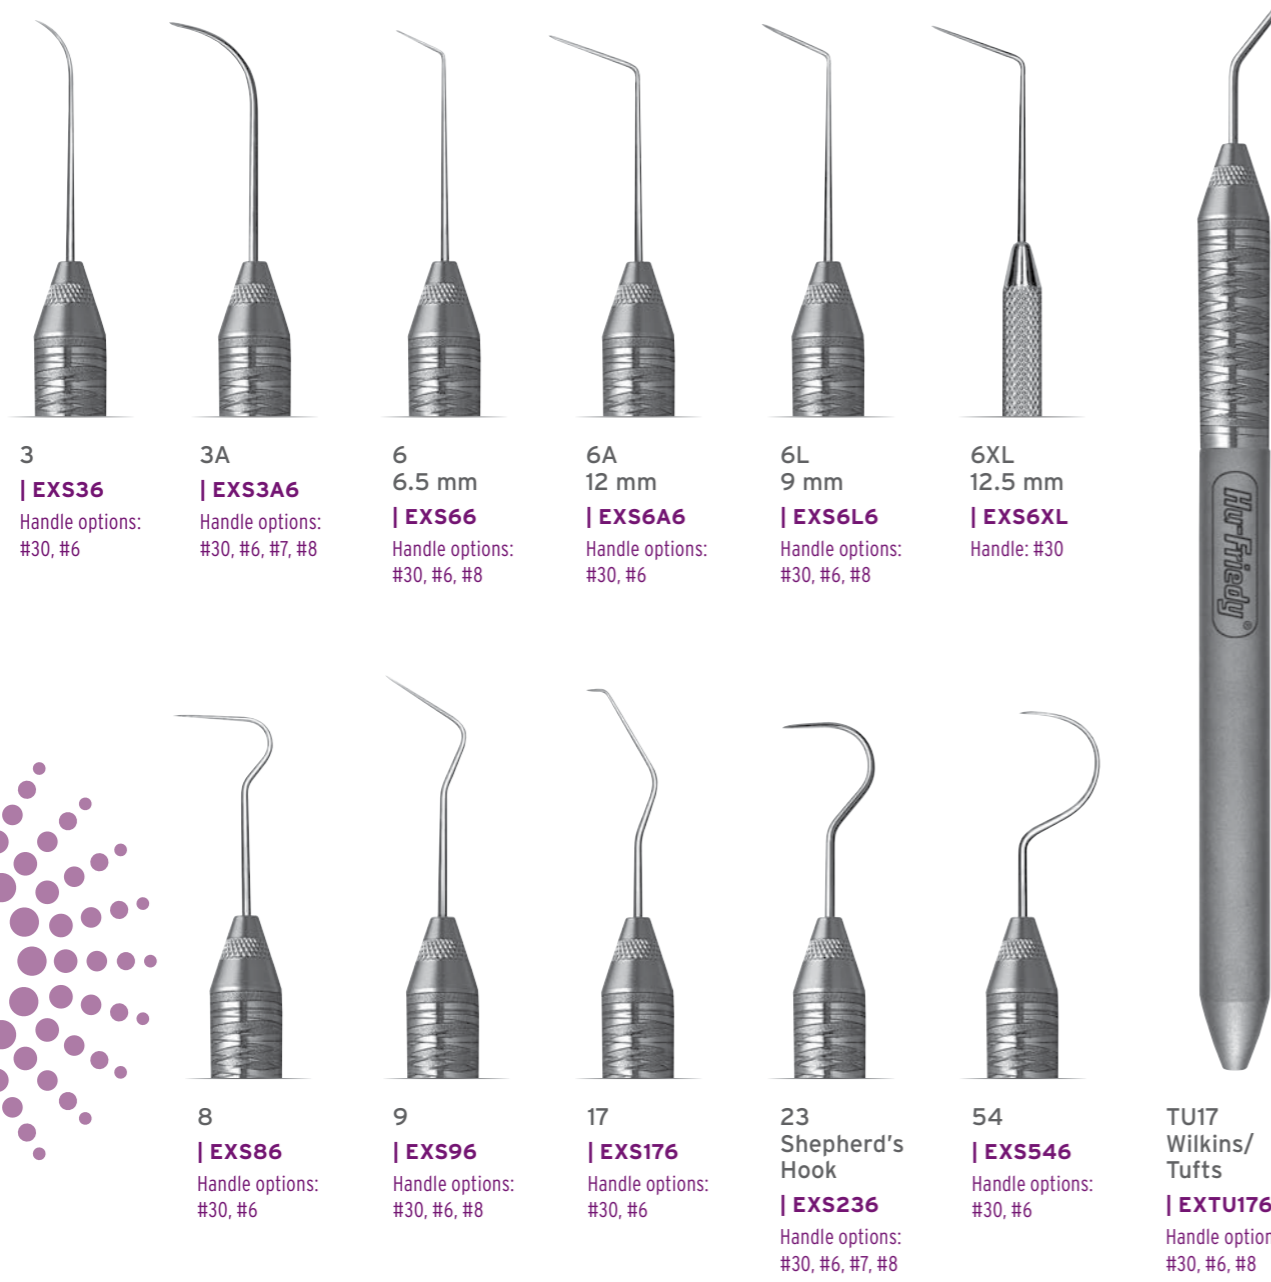

- 3** | EXS36
Handle options: #30, #6
- 3A** | EXS3A6
Handle options: #30, #6, #7, #8
- 6** 6.5 mm | EXS66
Handle options: #30, #6, #8
- 6A** 12 mm | EXS6A6
Handle options: #30, #6
- 6L** 9 mm | EXS6L6
Handle options: #30, #6, #8
- 6XL** 12.5 mm | EXS6XL
Handle: #30
- 8** | EXS86
Handle options: #30, #6
- 9** | EXS96
Handle options: #30, #6, #8
- 17** | EXS176
Handle options: #30, #6
- 23** Shepherd's Hook | EXS236
Handle options: #30, #6, #7, #8
- 54** | EXS546
Handle options: #30, #6
- TU17** Wilkins/Tufts | EXTU176
Handle options: #30, #6, #8

DOUBLE-END EXPLORERS

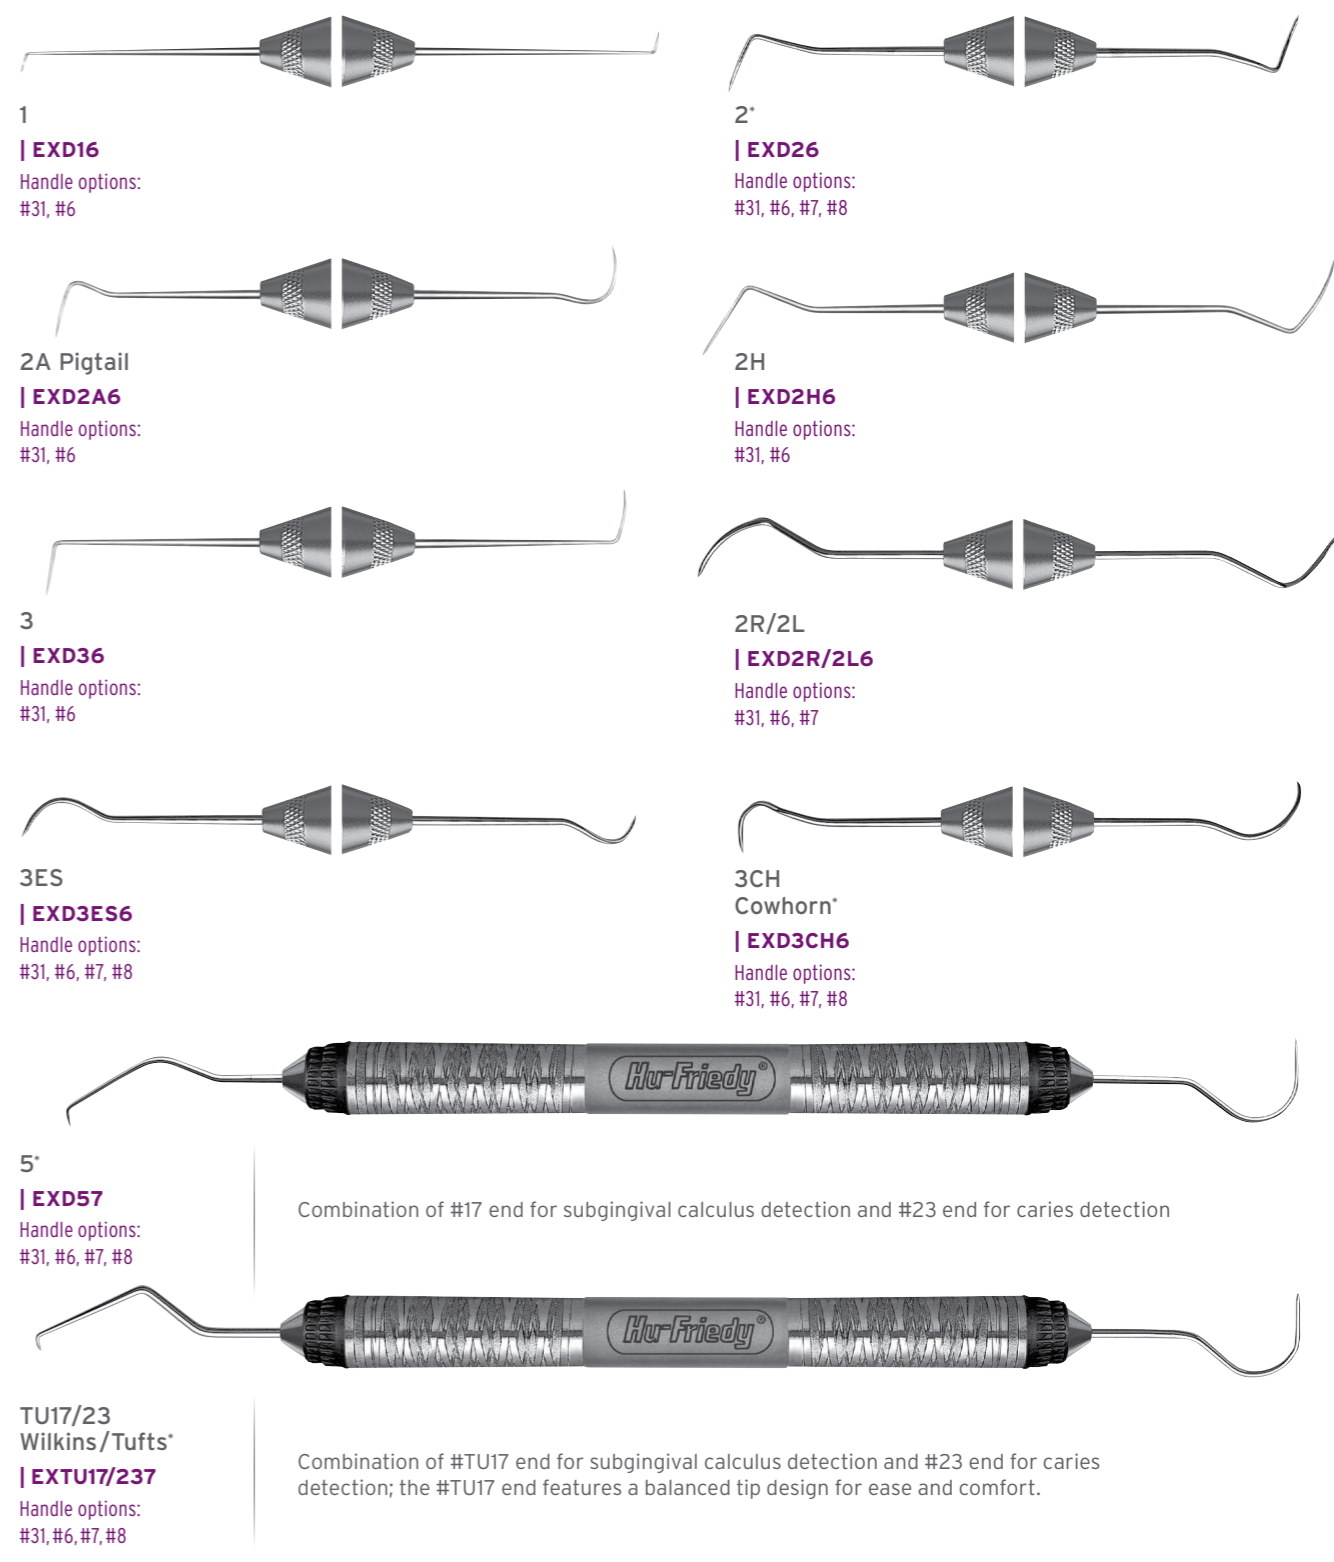

- 1** | EXD16
Handle options: #31, #6
- 2*** | EXD26
Handle options: #31, #6, #7, #8
- 2A Pigtail** | EXD2A6
Handle options: #31, #6
- 2H** | EXD2H6
Handle options: #31, #6
- 3** | EXD36
Handle options: #31, #6
- 2R/2L** | EXD2R/2L6
Handle options: #31, #6, #7
- 3ES** | EXD3ES6
Handle options: #31, #6, #7, #8
- 3CH** Cowhorn* | EXD3CH6
Handle options: #31, #6, #7, #8
- 5*** | EXD57
Handle options: #31, #6, #7, #8
- TU17/23** Wilkins/Tufts* | EXTU17/237
Handle options: #31, #6, #7, #8

Combination of #17 end for subgingival calculus detection and #23 end for caries detection

Combination of #TU17 end for subgingival calculus detection and #23 end for caries detection; the #TU17 end features a balanced tip design for ease and comfort.

*Explorers #2, #3CH, #5 and #TU17/23 are available with XTS coating (see page B5).


Hu-Friedy explorers are hand crafted from Duraspond™ steel, a specially blended steel alloy which provides flexibility and resilience for even the most precise diagnostic procedures.



DOUBLE-END EXPLORERS



To correctly adapt the tip of the 11/12 ODU explorer, place the tip interproximally so that the terminal shank is parallel to the tooth surface.

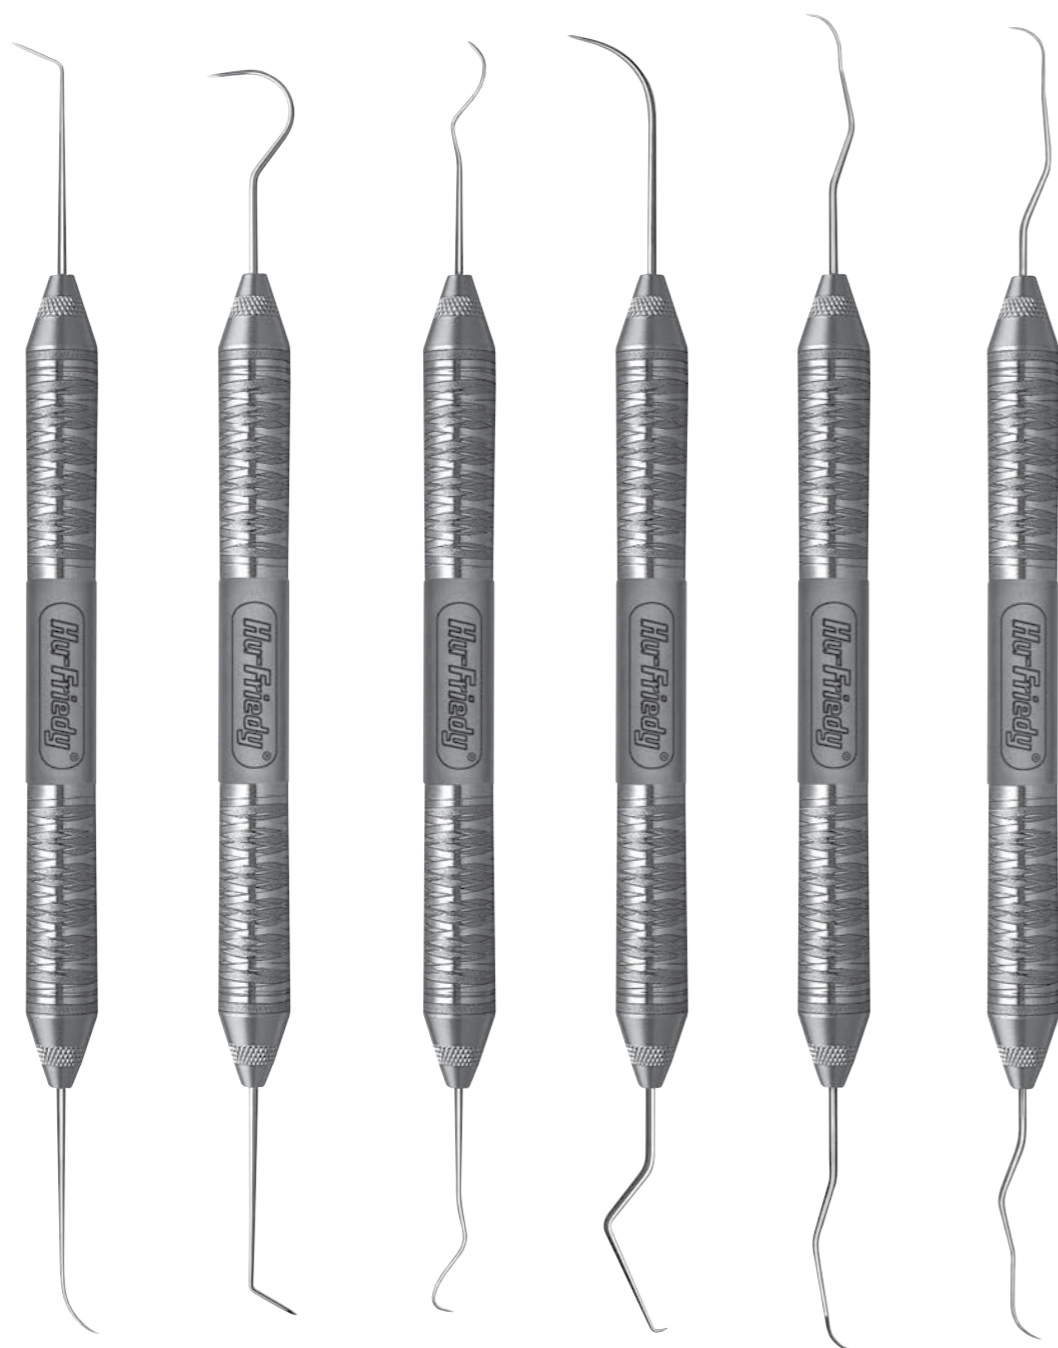

6/3
| **EXD66**
Handle options:
#31, #6
Combination of #6 and #3 explorers.

23/6
| **EX23/66**
Handle options:
#31, #6

EN1
| **EXDEN16**
Handle options:
#31, #6
For improved reach into interproximal areas.


3A/TU17
| **EX3A/TU176**
Handle options:
#31, #6

11/12
Old Dominion University
| **EXD11/126**
Handle options:
#31, #6, #7, #8
Ideal for posterior calculus detection in deep pockets, especially on proximal surfaces. Designed to explore an entire dentition with a single instrument.

11/12AF
After Five®
| **EXD11/12A6**
Handle options:
#31, #6, #7, #8
Similar to the EXD11/12 but 3 mm longer at the terminal shank for better access in deeper pockets.

SATIN STEEL® XTS® DOUBLE-END EXPLORERS

Satin Steel® XTS® explorers feature a non-stick Aluminum Titanium Nitride (AlTiN) coating.

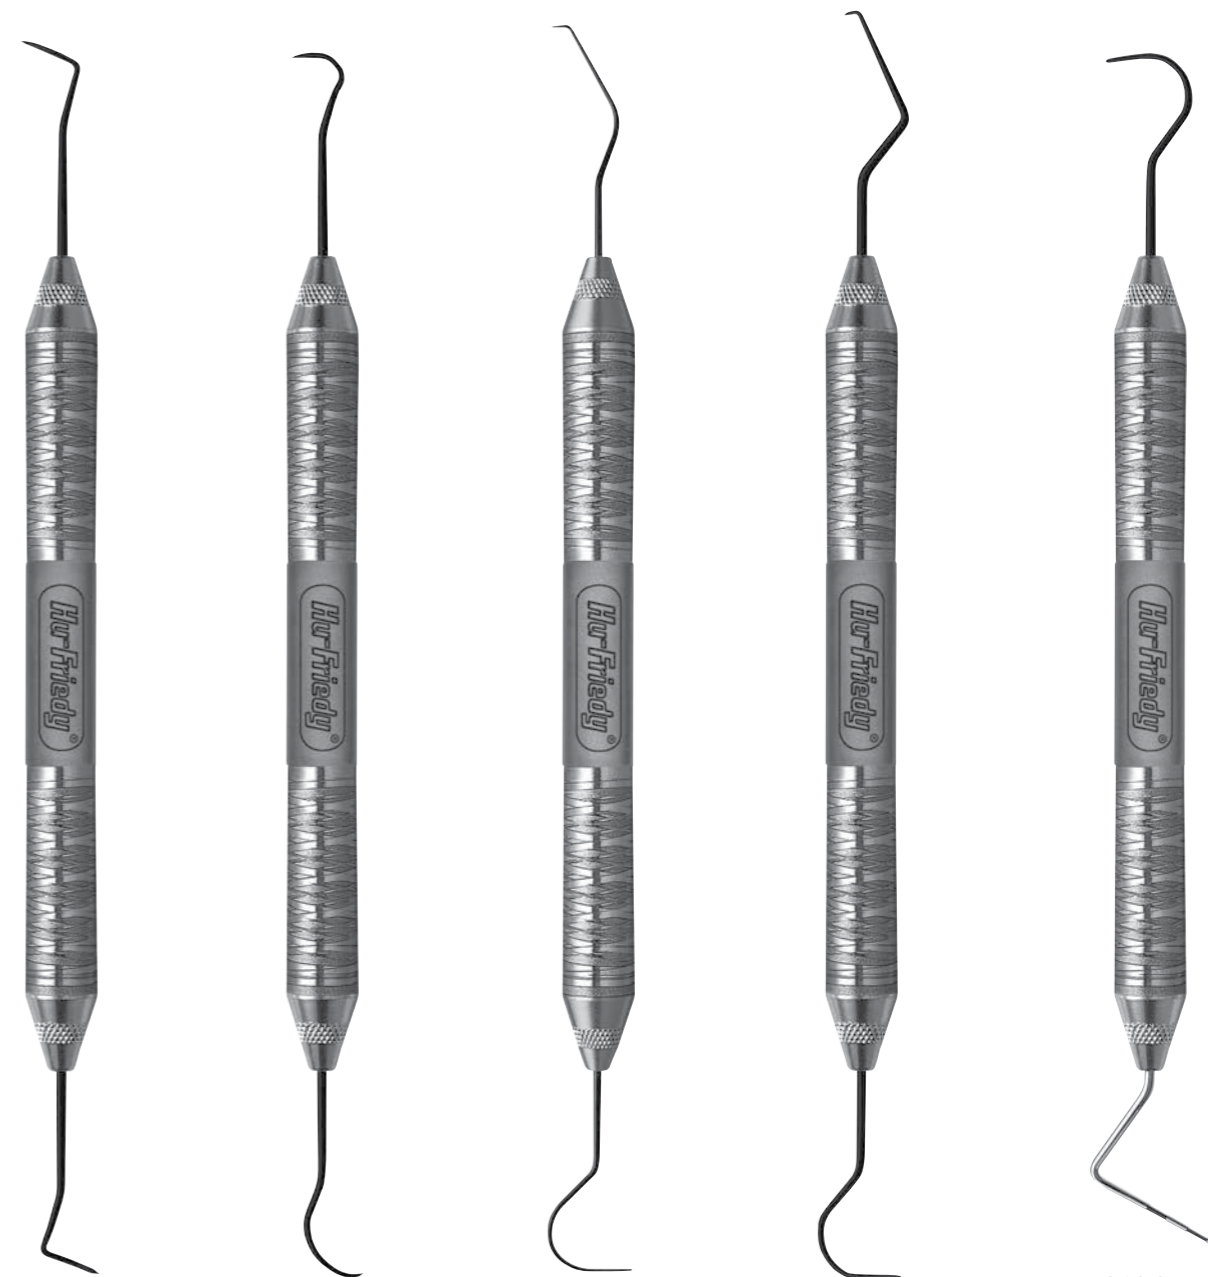

2
| **EXD2XTS**
Handle: #6

3CH
Cowhorn
| **EXD3CHXTS**
Handle: #6

5
| **EXD5XTS**
Handle: #6

TU17/23
Wilkins/Tufts
| **EXTU1723XT**
Handle: #6


23/CP-12
| **XP23/12XTS**
Handle: #6

3-6-9-12


Satin Steel XTS explorers are perfect for contouring dental anatomy during composite restorations. The dark coating also improves contrast between tooth and instrument tip.



PLASTIC PROBES

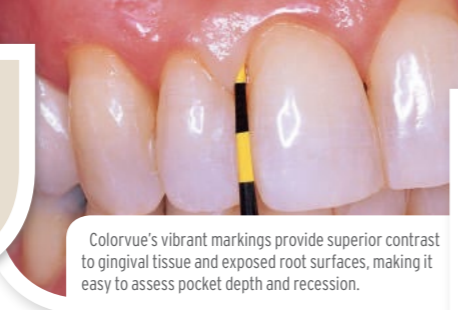

Colorvue's vibrant markings provide superior contrast to gingival tissue and exposed root surfaces, making it easy to assess pocket depth and recession.

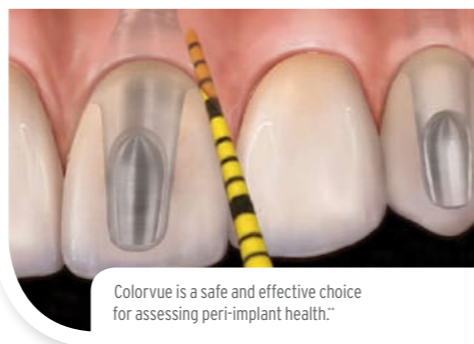

Colorvue is a safe and effective choice for assessing peri-implant health.**

COLORVUE® PROBES

Colorvue probes feature a vivid yellow tip with black markings for enhanced contrast to intraoral structures in both natural and implant dentition. Optimal flexibility and a rounded tip provide greater patient comfort and acceptability. The probe tips are safe for use with implants and feature a twist-on design for easy replacement of worn tips.



- 11**
3-6-8-11
| **PCV11PT**
12 Replacement Tips
| **PCV11KIT6**
6 Pack,
1 handle + 7 tips
| **PCV11KIT12**
12 Pack,
2 handles + 12 tips
- 12**
3-6-9-12
| **PCV12PT**
12 Replacement Tips
| **PCV12KIT6**
6 Pack,
1 handle + 7 tips
| **PCV12KIT12**
12 Pack,
2 handles + 12 tips
- Williams**
1-2-3-5-7-8-9-10
| **PCVWPT**
12 Replacement Tips
| **PCVWKIT6**
6 Pack,
1 handle + 7 tips
- UNC12**
1-2-3-4-5-6-7-8-9-10-11-12
| **PCVUNC12PT**
12 Replacement Tips
| **PCVNCKIT6**
6 Pack,
1 handle + 7 tips
| **PCVNCKIT12**
12 Pack,
2 handles + 12 tips



Colorvue Oxford Probe
| **PCVOKIT6**
Colorvue Oxford Starter Kit with 1 UNC15 probe/PH6 handle and 6 Colorvue UNC15 tips
| **PCVO12PT**
Refill Pack of Colorvue Oxford Tips

EXPRO HANDLES



17 Expro and Handle*
| **XP17/PH6**

23 Expro and Handle*
| **XP23/PH6**

TU17 Expro and Handle*
| **XPTU17/PH6**

*Colorvue PerioScreen tips sold separately.
**©Montage Media 2005. Excerpts from white paper on implant maintenance. Rethman M. Hu-Friedy Mfg. Co., LLC. September 2010.

COLORVUE® PERIOSCREEN® PROBES

Hu-Friedy's Colorvue PerioScreen probe provides a fast and easy-to-use method of screening periodontal pocket depth prior to definitive probing. A universally understood color-coding of green and red indicates the absence or presence of periodontal disease.



#10 Markings
3-5-7-10
| **PPS10PT**
12 Replacement Tips
| **PPS10KIT6**
6 Pack, 1 handle + 7 tips
| **PPS10KIT12**
12 Pack, 2 handles + 12 tips
| **PPSPROMO10**
Intro Kit: 1 handle + 1 tip

#12 Markings
3-6-9-12
| **PPS12PT**
12 Replacement Tips
| **PPS12KIT6**
6 Pack, 1 handles + 7 tips
| **PPS12KIT12**
12 Pack, 2 handles + 12 tips
| **PPSPROMO12**
Intro Kit: 1 handle + 1 tip

Colorvue Goldstein Probe
| **PPSGKIT6**
Kit 1 Handle + 7 Tips
| **PPSG12PT**
12 Replacement Tips

Colorvue®
| **PH6**

EXPRO HANDLES



17 Expro and Handle*
| **XP17/PH6**

23 Expro and Handle*
| **XP23/PH6**

TU17 Expro and Handle*
| **XPTU17/PH6**

*Colorvue PerioScreen tips sold separately.


Colorvue PerioScreen features a metal handle that is not only more ergonomic, but can also be reused or recycled. Only disposing of the plastic working end offers a "greener" instrumentation solution than other plastic probing systems.



METAL PROBES

QULIX™ COLOR-CODED PROBES

Qulix™ probes are color-coded with accurate, smoothly finished black markings which will not chip, flake or fade—ensuring you get a long lasting instrument for the best value!



2-4-6-8-10-12



CP2
| **PCP26**
Handle options:
#30, #6

3-6-8-11



CP-8
| **PCP86**
Handle options:
#30, #6

1-2-3-5-7-8-9-10



CP-10
| **PCP106**
Handle options:
#30, #6, #7, #8

3-6-8-11



CP-11
| **PCP116**
Handle options:
#30, #6, #7, #8

3-6-9-12



CP-12
| **PCP126**
Handle options:
#30, #6, #7, #8

3-5-8-10



CP-18
| **PCP186**
Handle options:
#30, #6, #8

1-2-3-4-5-6-7-8-9-10-11-12



CP-12
University of North Carolina
| **PCPUNC126**
Handle options:
#30, #6, #7, #8

1-2-3-4-5-6-7-8-9-10-11-12-13-14-15



CP-15
University of North Carolina
| **PCPUNC156**
Handle options:
#30, #6, #7, #8

3-6-8



PQ-O
Michigan
| **PQO6**
Handle options:
#30, #6

1-2-3-5-7-8-9-10



PQ-W
Williams
| **PQW6**
Handle options:
#30, #6, #7, #8

1-2-3-5-7-8-9-10



PQ-OW*
Thin Williams
| **PQOW6**
Handle options:
#30, #6, #7, #8

1-2-3-5-7-8-9-10



Maryland
Laser Etched
| **PCPMDBIU**
Handle: #30

3.5-5.5-8.5-11.5




CP-11.5B*
Screening Probe
| **PCP11.5B6**
Handle options:
#30, #6, #7, #8

Hu-Friedy WHO style probes are perfect for successfully implementing PSR and CPITN periodontal screenings. Accurate color band from 3.5 mm to 5.5 mm and separate bands at 8.5 mm and 11.5 mm meets PSR criteria for accurate assessment of pockets.

*Michigan "O" with Williams markings

SINGLE-ENDED PROBES

Used to assess periodontal pocket depths, attachment levels, anatomy configurations and gingival bleeding


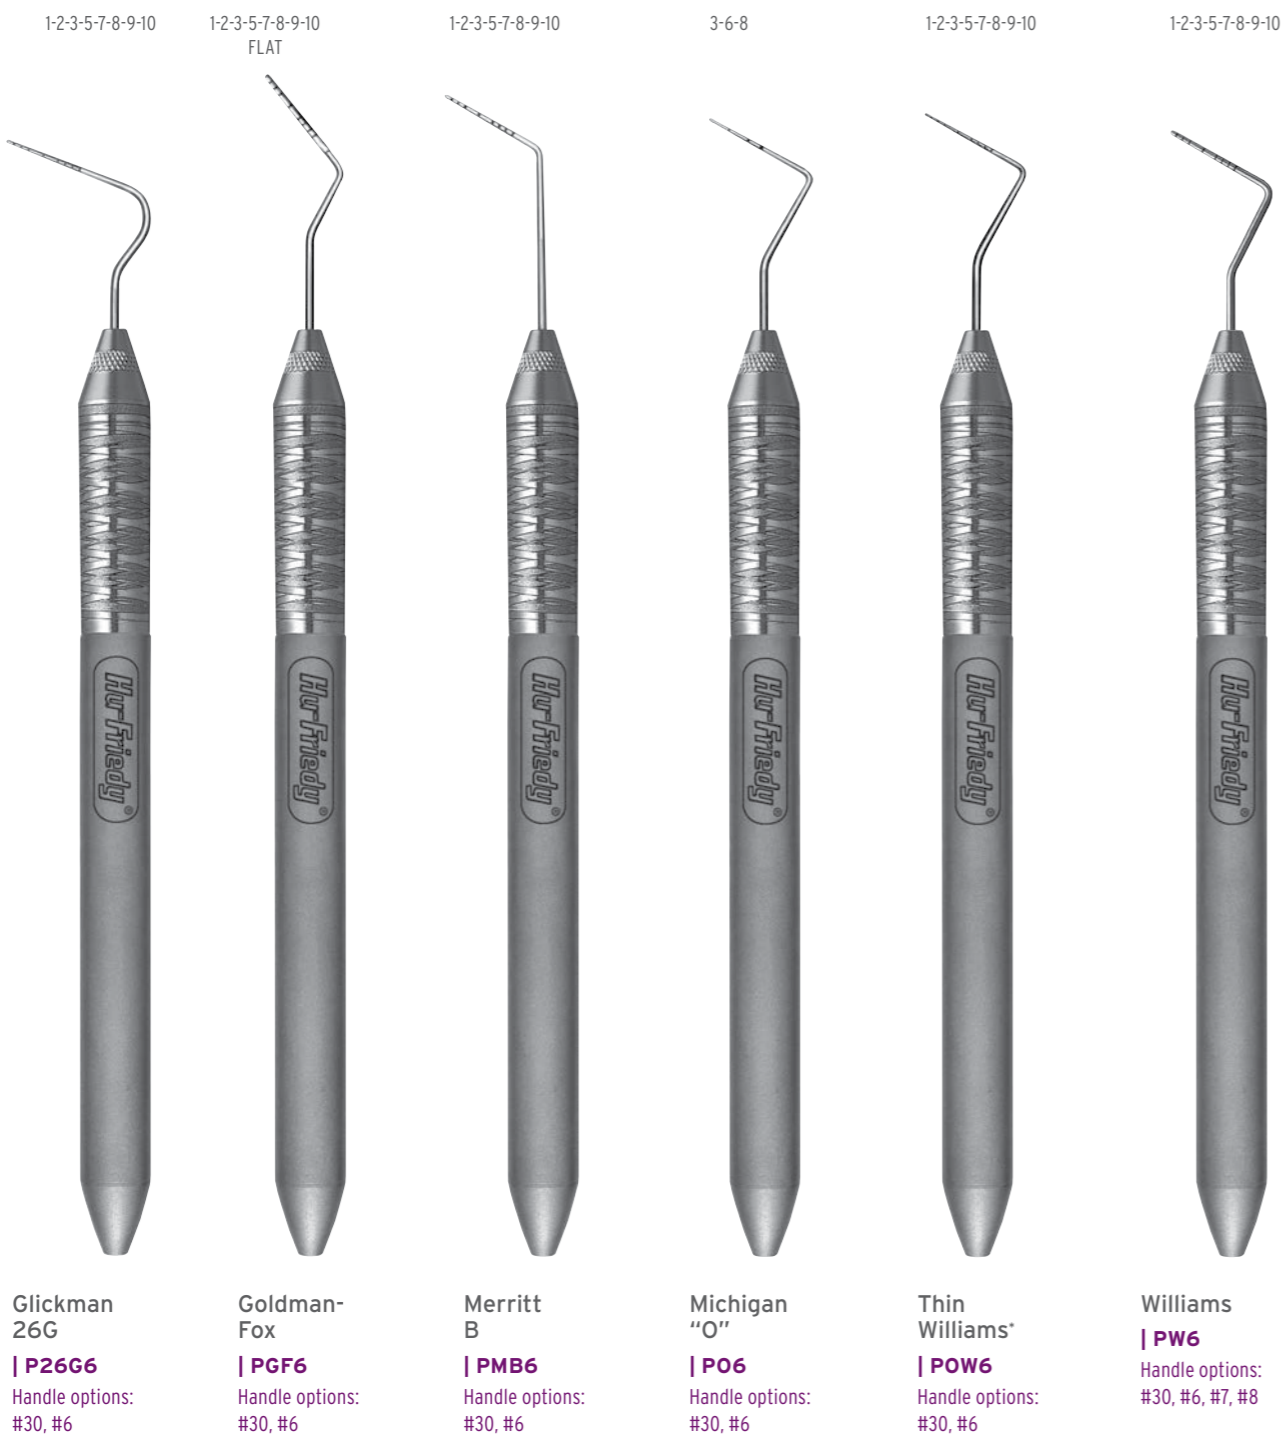


*Michigan "O" with Williams markings

Goldman-Fox probes feature a flat working end for easier insertion on lingual or facial surfaces.

NOVATECH™ PROBES


Unique right angle design for improved adaptability in posterior regions.

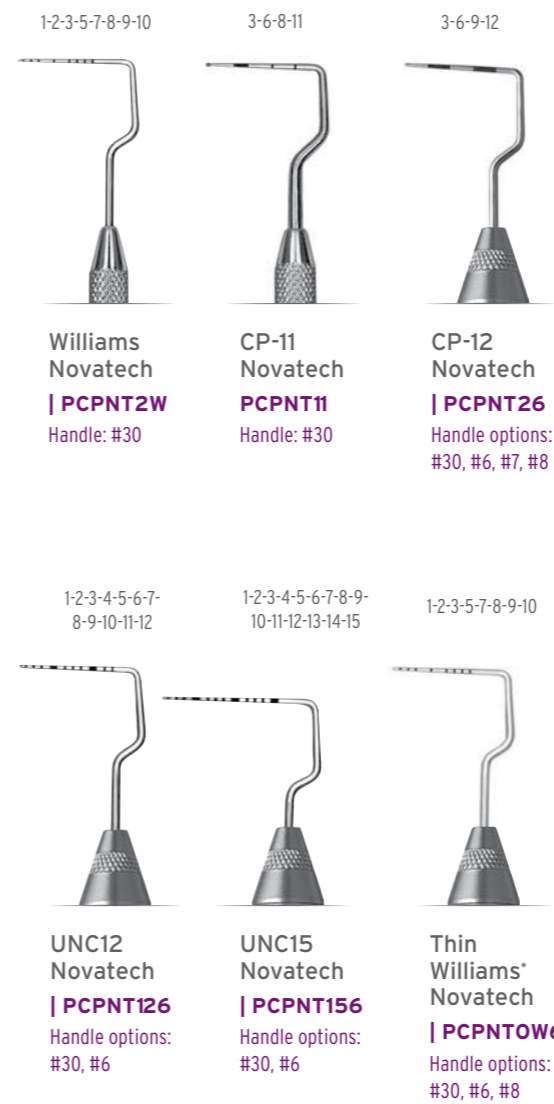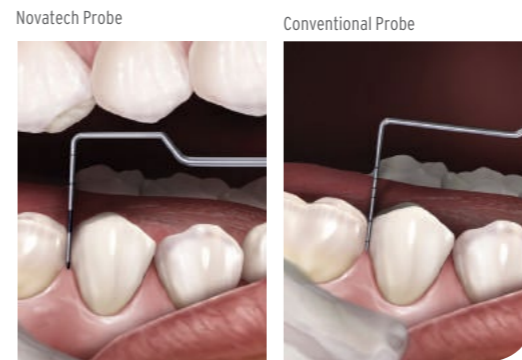

*Michigan "O" with Williams markings

**Hu-Friedy's WHO style Probe used with PSR and CPITN periodontal screening programs

DOUBLE-ENDED SCREENING PROBES

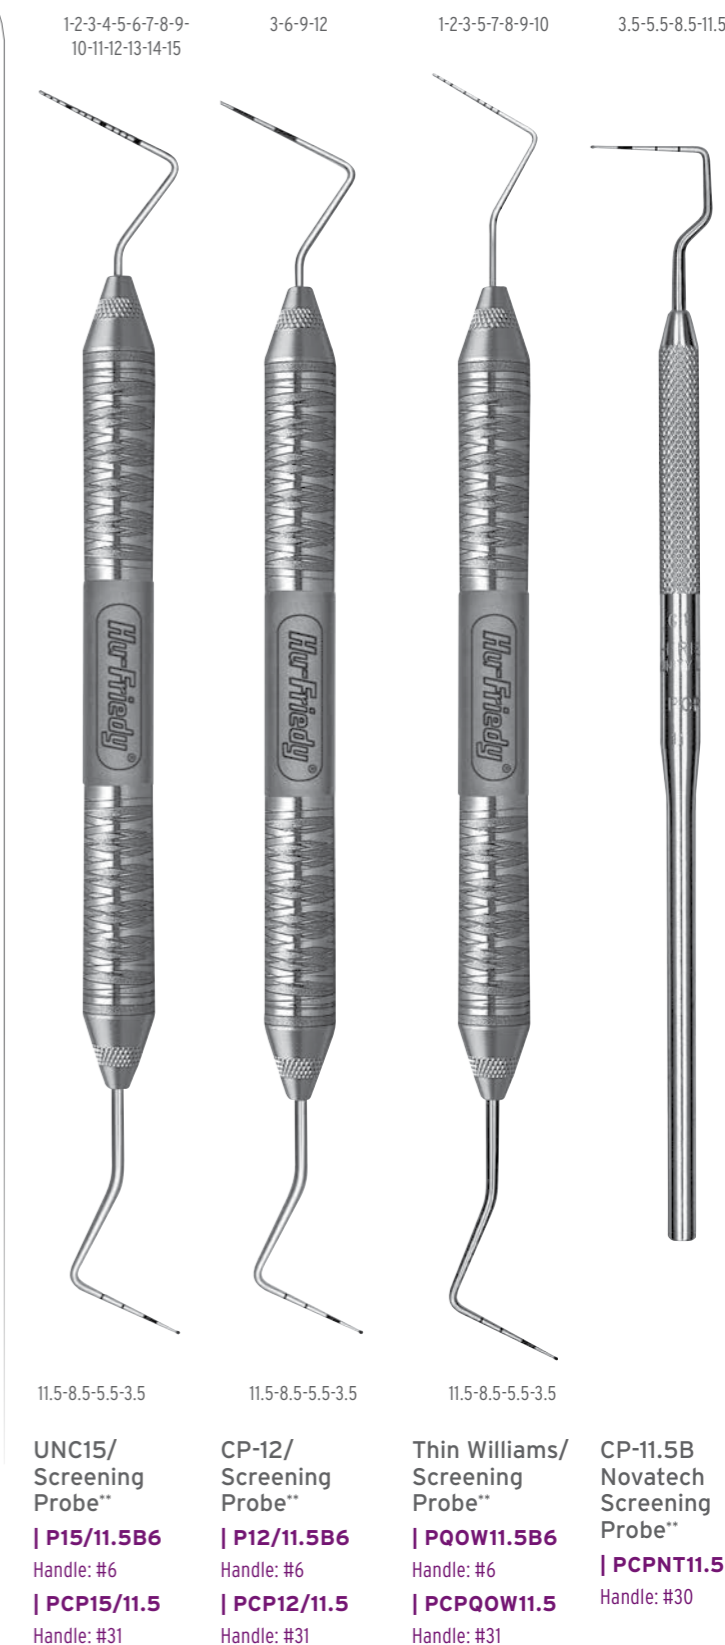




METAL PROBES

DOUBLE-ENDED

3-6-9-12 1-2-3-5-7-8-9-10 FLAT 1-2-3-5-7-8-9-10 FLAT 1-2-3-5-7-8-9-10 FLAT 1-2-3-5-7-8-9-10 3-6-9-12

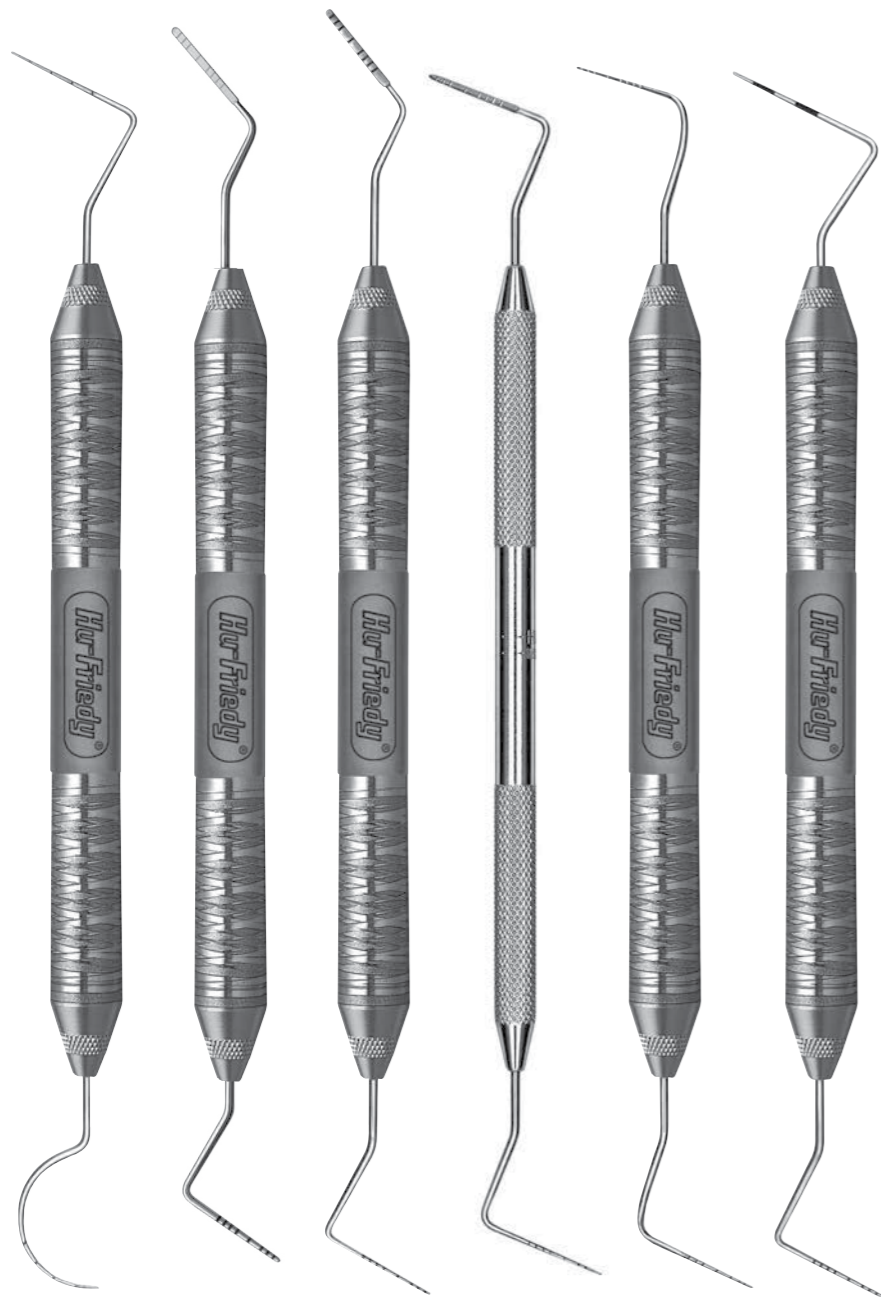

12-9-6-3 10-9-8-7-5-3-2-1 10-9-8-7-5-3-2-1 10-9-8-7-5-3-2-1 FLAT 10-9-8-7-5-3-2-1 10-9-8-7-5-3-2-1


- UT3/4 Cattoni**
| **P3/46**
Handle options: #31, #6
- Goldman-Fox Williams**
| **PGF/W6**
Handle options: #31, #6, #7, #8
- Goldman-Fox Williams Laser-etched**
| **PCPGF/W6**
Handle options: #31, #6
- 3N Nabers**
| **P3N**
Handle: #31
- Williams DE Offset**
| **PWD6**
Handle options: #31, #6
- CP-12/Thin Williams***
| **PCP12/QOW6**
Handle: #6

DOUBLE-ENDED FURCATION PROBES

Color-coded Nabers probe in 1st molar furcation.



3-6-9-12

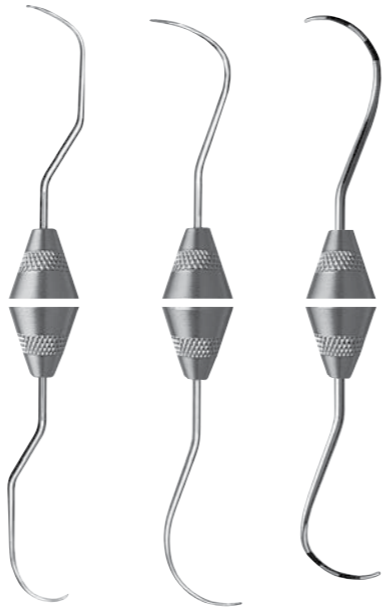

12-9-6-3

- 1N Nabers**
| **P1N6**
Handle options: #31, #6
- 2N Nabers**
| **P2N6**
Handle options: #31, #6
- Q-2N Nabers Color-coded**
| **PQ2N6**
Handle options: #31, #6, #7, #8

*Michigan "0" with Williams markings



EXPROS

A double-ended instrument that combines two critical instruments required for every effective diagnostic set-up—with an explorer on one end and a probe on the other, an Expro is excellent for dental examinations and charting.




10-9-8-7-5-3-2-1 10-9-8-7-5-3-2-1 11-8-6-3

- 23/QW Williams**
| **XP23/QW6**
Handle options: #31, #6
- 23/QOW* Thin Williams**
| **XP23/QOW6**
Handle options: #31, #6, #7, #8
- 23/CP-8**
| **XP23/86**
Handle options: #31, #6


*Wilkins/Tufts University of North Carolina

*Michigan "0" with Williams markings

**Hu-Friedy's WHO style Probe used with PSR and CPITN periodontal screening programs

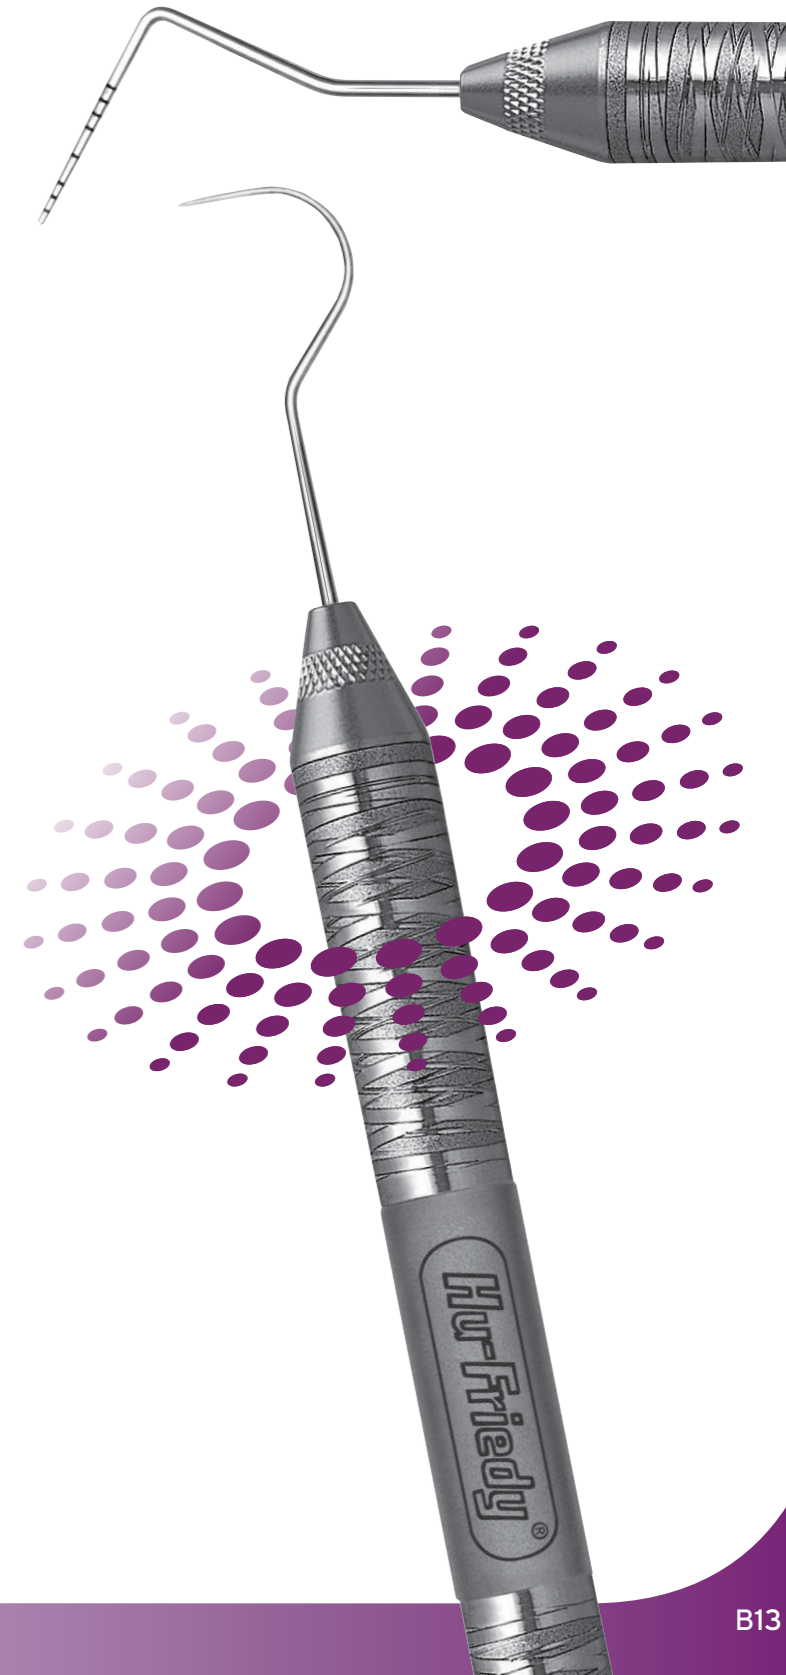

Hu-Friedy®

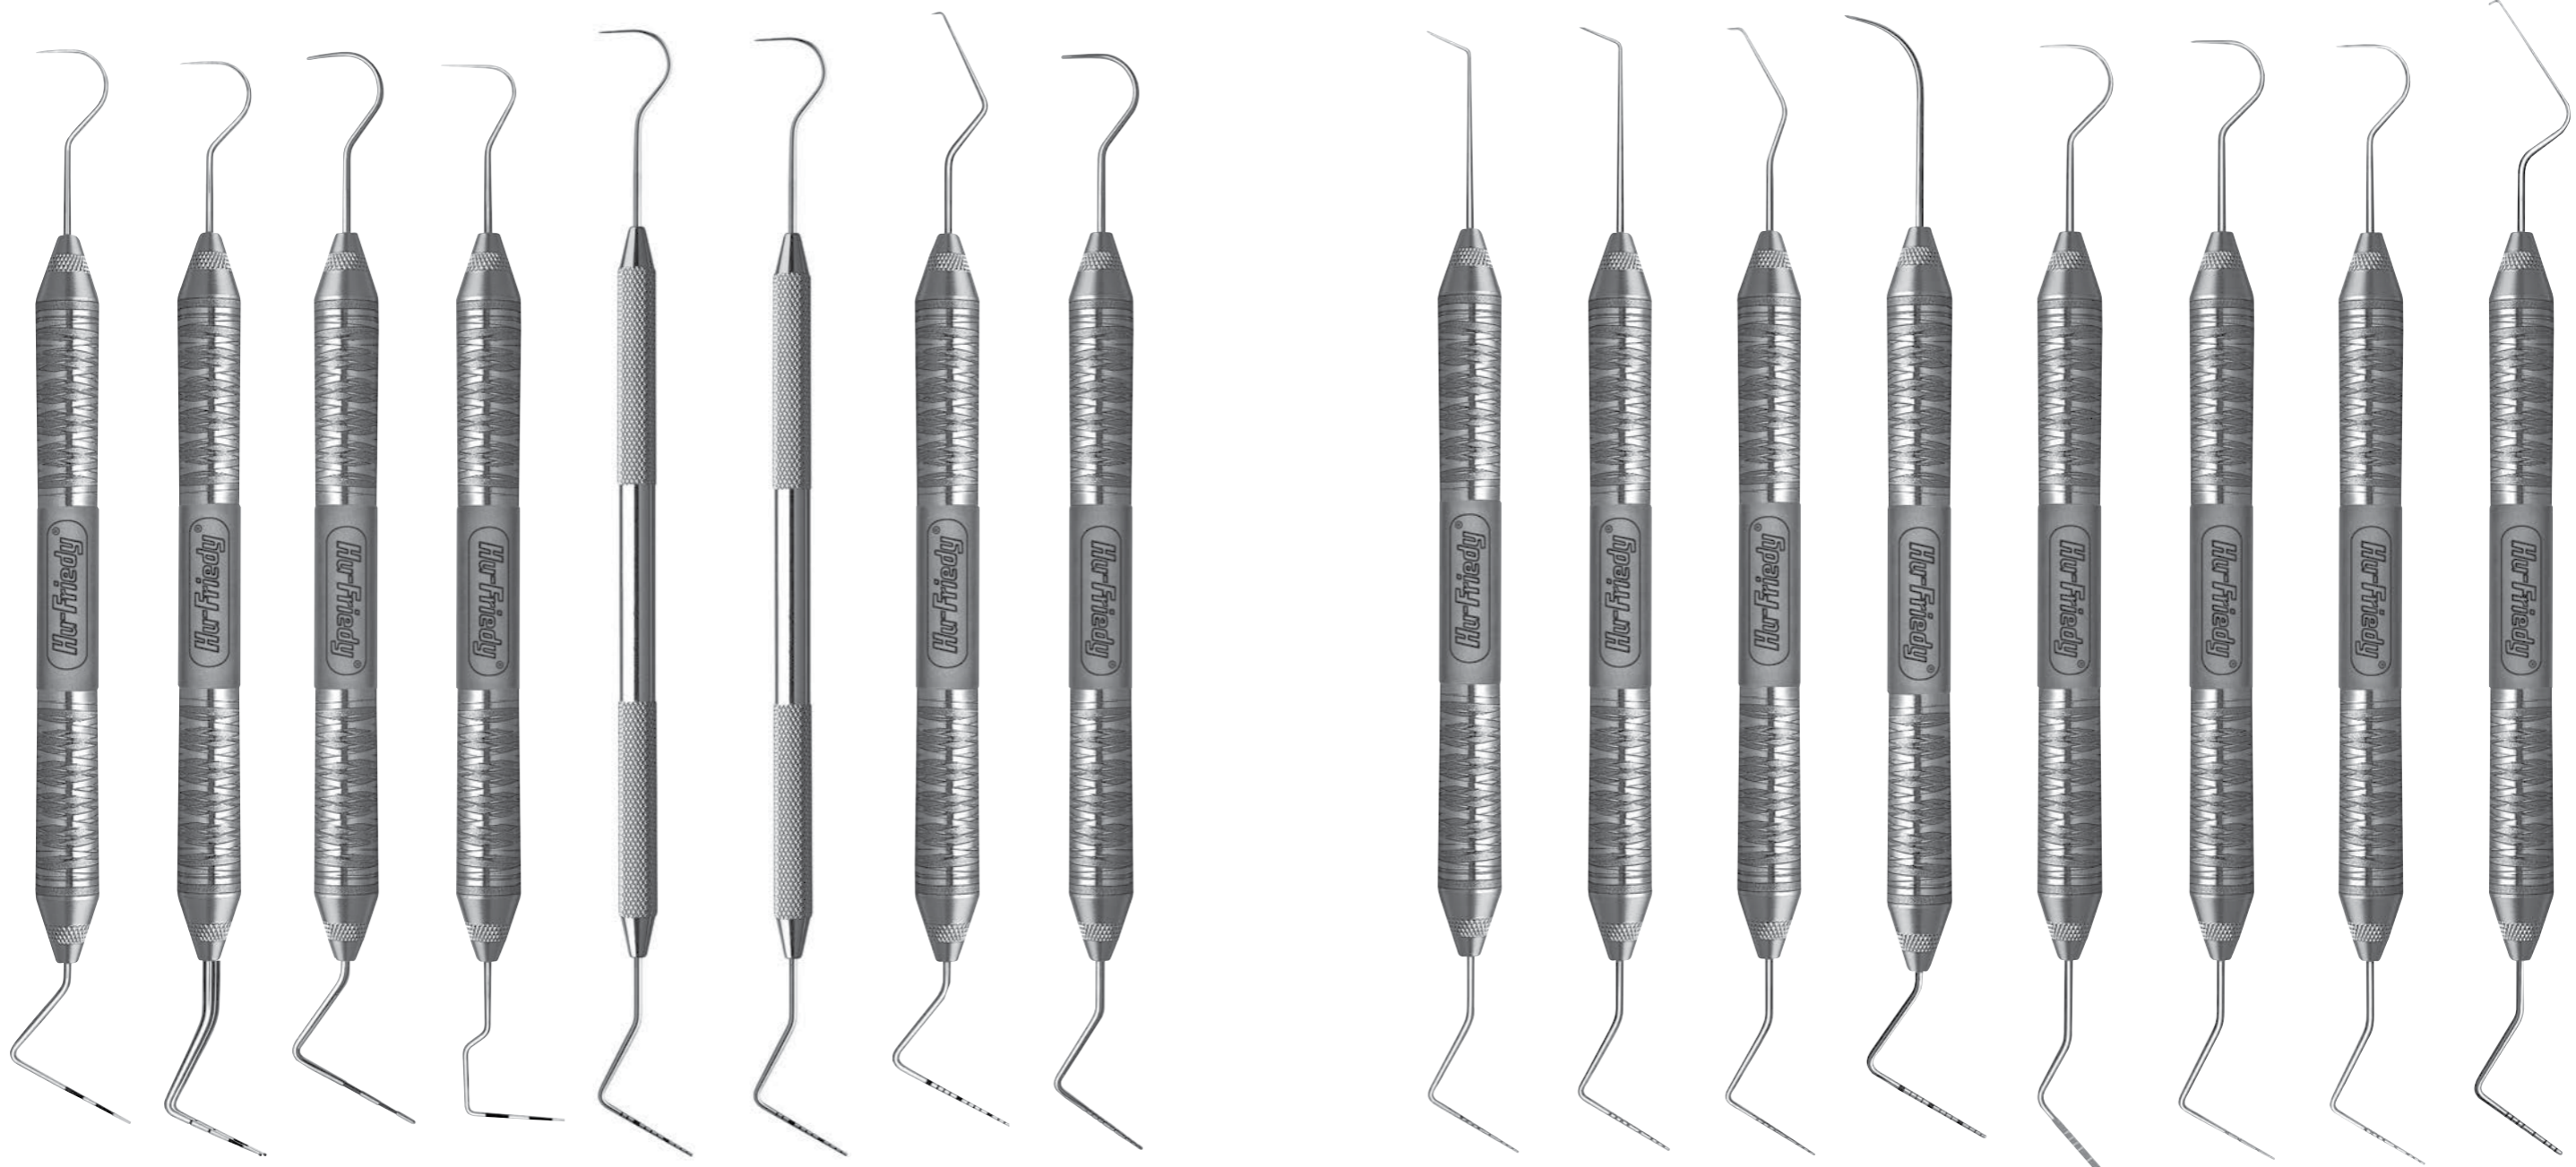

11-8-6-3 11.5-8.5-5.5-3.5 12-9-6-3 12-9-6-3 12-11-10-9-8-7-6-5-4-3-2-1 15-14-13-12-11-10-9-8-7-6-5-4-3-2-1 15-14-13-12-11-10-9-8-7-6-5-4-3-2-1 10-9-8-7-5-3-2-1 10-9-8-7-5-3-2-1 10-9-8-7-5-3-2-1 10-9-8-7-5-3-2-1 15-14-13-12-11-10-9-8-7-6-5-4-3-2-1 10-9-8-7-5-3-2-1 FLAT 8-6-3 10-9-8-7-5-3-2-1 10-9-8-7-5-3-2-1

<p>23/CP-11 XP23/116 Handle options: #31, #6</p>	<p>23/CP-11.5B Screening Probe™ XP23/126 XP23/11.56 Handle options: #31, #6, #7, #8</p>	<p>23/CP-12 XP23/126 Handle options: #31, #6, #7, #8</p>	<p>NT3/CP-12 Novatech XPNT36 Handle options: #31, #6</p>	<p>23/UNC12 University of North Carolina XP23/UNC12 Handle: #31 XP23/NC12 Handle: #6 XP23/NC127 Handle: #7 XP23/NC128 Handle: #8</p>	<p>23/UNC15 University of North Carolina XP23/UNC15 Handle: #31 XP23/UNC6 Handle: #6 XP23/UNC7 Handle: #7 XP23/UNC8 Handle: #8</p>	<p>TU17/UNC15* XPTU17/15 Handle options: #31, #6</p>	<p>23/W Williams XP23/W6 Handle options: #31, #6, #7, #8</p>	<p>6/OW* Thin Williams XP6/OW6 Handle options: #31, #6</p>	<p>6/W Williams XP6/W6 Handle options: #31, #6</p>	<p>17/OW* Thin Williams XP17/OW6 Handle options: #31, #6</p>	<p>3A/UNC15 XP3A/UNC15 Handle options: #31, #6</p>	<p>23/GF Goldman- Fox XP23/GF6 Handle options: #31, #6</p>	<p>23/O Michigan XP23/O6 Handle options: #31, #6</p>	<p>23/OW* Thin Williams XP23/OW6 Handle options: #31, #6</p>	<p>20F/QOW* Thin Williams XP20F/QOW6 Handle options: #31, #6</p>
--	--	--	--	---	---	--	--	--	--	--	--	--	--	--	--



*Michigan "O" with Williams markings

*Michigan "O" with Williams markings



DRESSING PLIERS

Used to grasp or transfer materials in and out of the oral cavity, all dressing pliers are made of heavy-gauge, heat-treated stainless steel to prevent tip bending and misalignment.

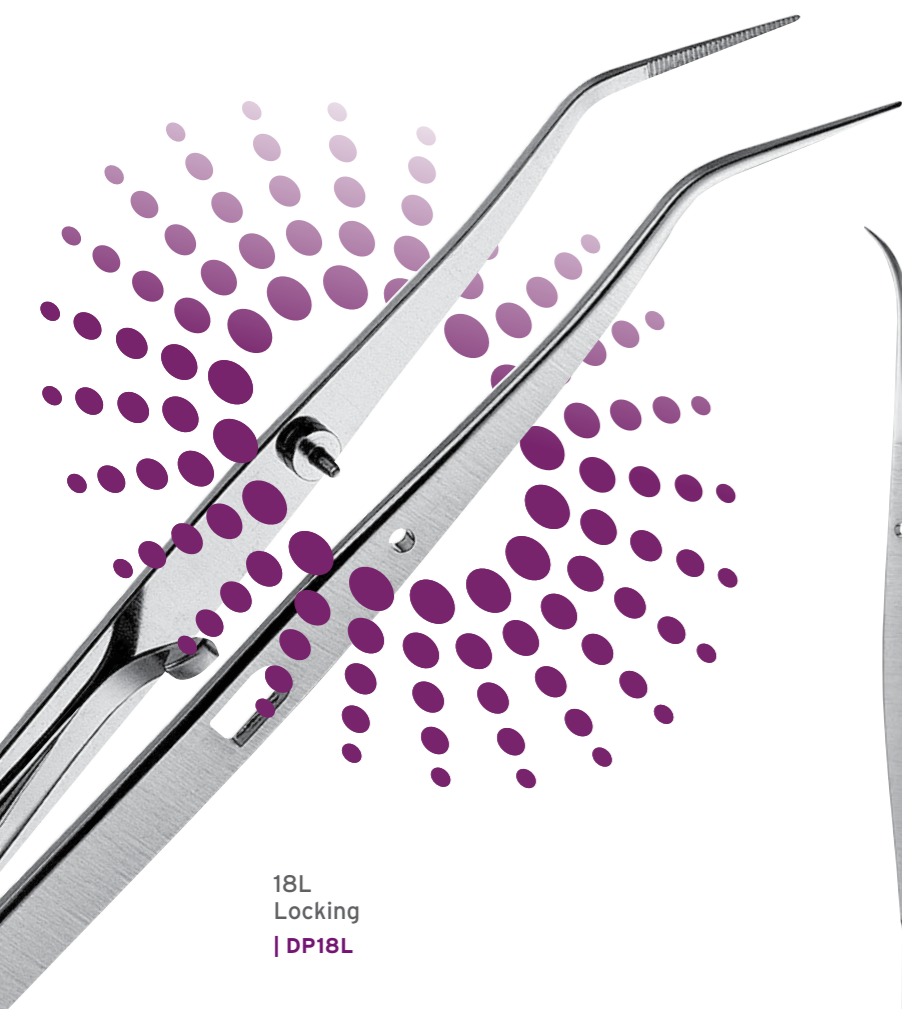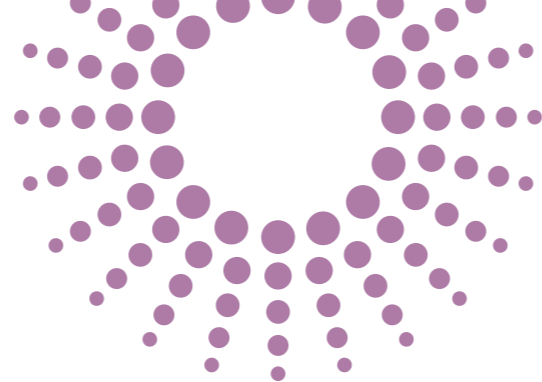

18L
Locking
| DP18L



1 Perry
| DP1



2 College
| DP2



3
| DP3



17
| DP17



18
| DP18



19
| DP19



Utility
Pick-Up
Dressing Pliers
| DPU17



317
Smooth
Beak
| DP317



318
Foil/Meriam
Serrated Beak
| DP318

Use of the DPU17 Utility Dressing Pliers for transporting contaminated/soiled objects; cotton gauze squares, rubber dam material, carbon burs, etc., at chairside or in the sterilization area can reduce the risk of cross-contamination.


DP317 Dressing Pliers feature non-serrated beaks making them ideal for the placement of antimicrobial chips.





HIGH DEFINITION MIRRORS

Hu-Friedy's new High Definition Mirrors feature a proprietary coating that provides superior brilliance and color for increased visibility in all dental procedures. Also scratch-resistant, our HD mirrors are the clear choice for optimal patient treatment.

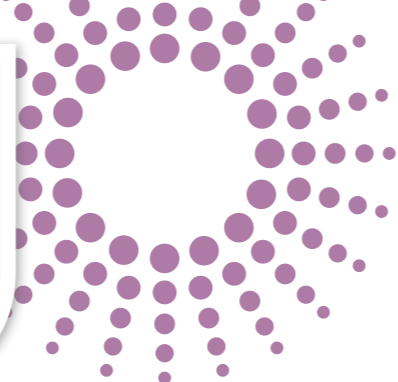

CONE SOCKET



#3 Single-Sided
| **MIR3HD**
Single



#4 Single-Sided
| **MIR4HD**
Single
| **MIR4HD3**
Box of 3
| **MIR4HD12**
Box of 12



#5 Single-Sided
| **MIR5HD**
Single
| **MIR5HD3**
Box of 3
| **MIR5HD12**
Box of 12



#4 Double-Sided
| **MIR4DSHD**
Single
| **MIR4DSHD6**
Box of 6



#5 Double-Sided
| **MIR5DSHD**
Single
| **MIR5DSHD6**
Box of 6

EUROPEAN SIMPLE STEM



#3 Single-Sided
| **MIR3HDE**
Single



#4 Single-Sided
| **MIR4HDE**
Single
| **MIR4HDE3**
Box of 3
| **MIR4HDE12**
Box of 12



#5 Single-Sided
| **MIR5HDE**
Single
| **MIR5HDE3**
Box of 3
| **MIR5HDE12**
Box of 12



#4 Double-Sided
| **MIR4DSHDE**
Single
| **MIR4DSHDE6**
Box of 6



#5 Double-Sided
| **MIR5DSHDE**
Single
| **MIR5DSHDE6**
Box of 6

EUROPEAN SIMPLE STEM



Single-Sided #4'
7/8" (22 mm)
Diameter
| **M4C**
Box of 12



#4 Double-Sided
| **M4DC**
Box of 6



Single-Sided #5'
15/16" (24 mm)
Diameter
| **M5C**
Box of 12



#5 Double-Sided
| **M5DC**
Box of 6

PHOTOGRAPHY MIRRORS



1-1/2" Exam Mirror
with Handle**
| **M7H**



2" Exam Mirror
with Handle**
| **M8H**

RHODIUM MIRRORS

Rhodium-coated to resist scratching, Hu-Friedy's front surface mirrors provide sharp and distortion free images with a smooth finish for patient comfort. Available in both Cone Socket and European Simple Stem designs.



CONE SOCKET MIRRORS



Single-Sided #4
7/8" (22 mm)
Diameter
| **MIR4/3**
Box of 3
| **MIR4/12**
Box of 12



Double-Sided #4
7/8" (22 mm)
Diameter
| **MIR4DS/3**
Box of 3
| **MIR4DS/6**
Box of 6



Single-Sided #5
15/16" (24 mm)
Diameter
| **MIR5/3**
Box of 3
| **MIR5/12**
Box of 12



Double-Sided #5
1-5/16" (24 mm)
Diameter
| **MIR5DS/3**
Box of 3
| **MIR5DS/6**
Box of 6



High Definition Mirrors are 38.5% brighter than rhodium and feature a 113% reflection factor.*

*data on file

The ergonomic and stream-lined design of the double-sided mirror allows for maximum patient comfort and efficient cleaning due to crevice-free construction.

*Available only in Europe
**Not shown to size



MIRROR HANDLES

CONE SOCKET MIRROR HANDLES



#24
Cone
Socket
Mirror
Handle
| MH24

#1
Cone
Socket
Mirror
Handle
| MH1

#6
Cone
Socket
Mirror
Handle
| MH6

#7
Cone
Socket
Mirror
Handle
| MH7

#8
Cone
Socket
Mirror
Handle
| MH8

SIMPLE STEM MIRROR HANDLES



#6
Simple
Stem Mirror
Handle*
| MHE6

#7
Simple
Stem Mirror
Handle*
| MHE7

Round
Simple
Stem Mirror
Handle
| MH0175E



The blunt end of the mirror handle is ideal for testing sensitivity to percussion and assessing tooth mobility.